

## B-510 Series



**Advanced Routine Lab Upright Microscopes**

# Born To Be Professional

## HIGH-GRADE CONFIGURATIONS FOR PROFESSIONALS

- » Wide range to fulfill specific lab requirements
- » Valuable solutions for life and material sciences
- » Compliant with several observation methods

## AN AFFORDABLE PARTNER WITH HIGH-END FEATURES

- » IOS W-PLAN objectives for flat images on 22 mm FN
- » Full Koehler illumination for enhanced images
- » Rounded edge, rackless stage to prevent scratches



# Optically Impressive

## MAINTAINING GOOD EYESIGHT

- » 10x/22 eyepieces for large specimen view
- » Comfortable rubber cup to get rid of annoying external light
- » High eye-point for glasses wearers, dioptic adjustment (left eyepiece)

## B-510 & IOS W-PLAN: THE PERFECT COMBINATION

- » IOS Infinity corrected optical system
- » Full planarity optics on 22 mm (W-PLAN) according to ISO 19012-1
- » High-grade Semi-Apo lens available ideal for fluorescence





# An Extensive Range of Different Configurations

## THE MODELS FOR ASBESTOS TESTING IN ENVIRONMENTAL MONITORING

- » B-510ASB measures fiber concentrations in air and includes 40xPH lens and 12.5x Walton & Beckett eyepieces
- » B-510POL & B-510POL-I for bulk/fiber class identification

## B-510DK - THE DEDICATED MODEL FOR FRESH BLOOD ANALYSIS

- » Exclusive X-LED<sup>3</sup> darkfield cardioid condenser with high N.A. 1.36 and the new IOS W-PLAN 100x oil iris objective
- » Brightfield condenser also supplied

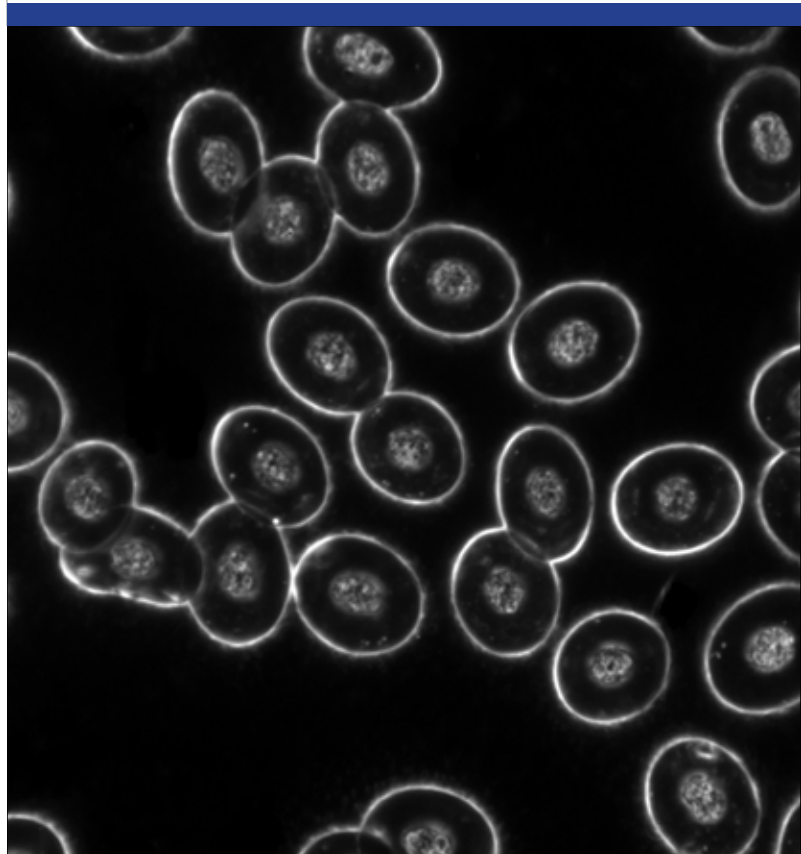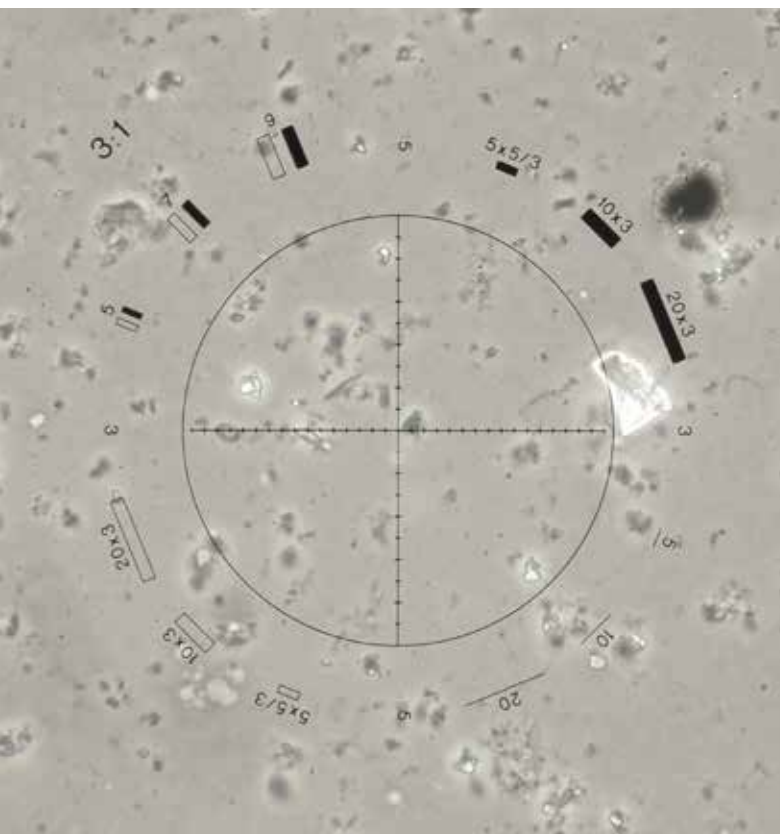

## Multiple Observation Methods

**BRIGHTFIELD**


**METALLOGRAPHY**

**DARKFIELD**

**POLARIZATION**

**FLUORESCENCE**

**PHASE CONTRAST**

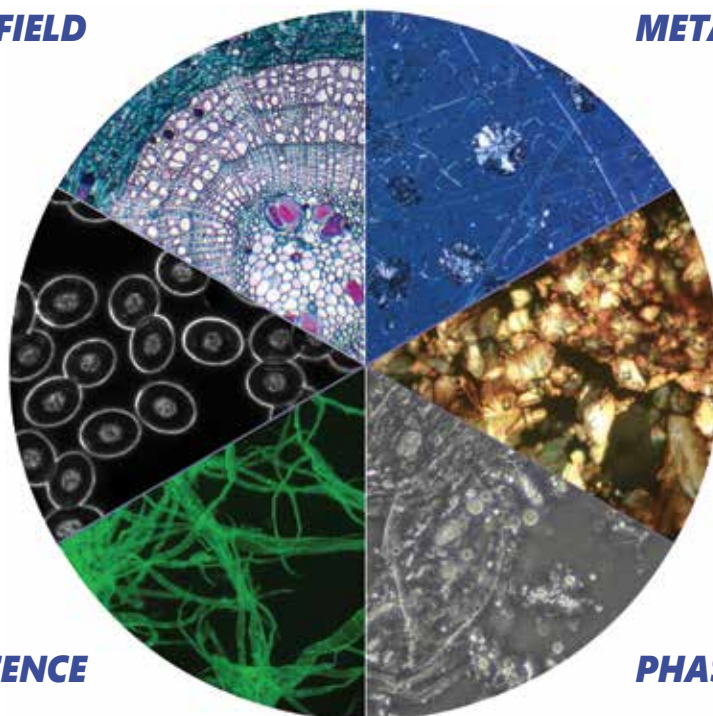

# Many Specimens, Many Observers - Intense Productivity

2

## INCREASE YOUR SAMPLE THROUGHPUT

- » Large, resistant stage to easily and quickly process 2 samples
- » Ergonomic design and controls for extended operation
- » Convenient handle for easy transportation

## DISCUSSION BRIDGES FOR SIMULTANEOUS OBSERVATIONS AND TEACHING

- » RGB pointer with brightness adjustment for the main observer
- » Face-to-face attachment with 1 extra viewing head, 20mm FN
- » Side attachment with 1, 2 & 4 extra viewing heads, 20mm FN

Laboratory



### **Multi-Head Discussion Microscopes**

With discussion bridges, up to 5 people/colleagues can observe the same image on B-510. Ideal for teaching and training students, especially in the medical field. The main observer and additional viewers will benefit of an extremely homogeneous light conditions, with a three-colour pointer with settable intensity to highlight points of interest.

# X-LED<sup>3</sup> - Only Available at OPTIKA

## STATE-OF-THE-ART ILLUMINATION SYSTEM

- » Uncomparable light intensity, exclusive lens & collector design
- » Constant pure-white color temperature at all intensity levels
- » Unmatched color fidelity, uniformity and brightness


## CUT ELECTRICITY BILLS BY 90%

- » Money & energy saving, only 3.6 W
- » More efficient brightness than a 50 W halogen lamp
- » LED long lifetime (65,000 hours = 22 years at 8 hours/day usage)



Halogen

X-LED<sup>3</sup>



Multi-plug power supply

# Go Digital - Vivid Colors & Contrast For Stunning Images

2

## STAY CONNECTED WITH YOUR SPECIMEN, EASILY

- » Trinocular port to be always updated with the latest technology cameras, even in the future
- » Wide range of cameras matching all the needs, including the more specific ones
- » Modern C-mount focusable professional adapters for all kinds of cameras

## PROFESSIONAL IMAGE ANALYSIS

- » Multi-language software for live-view, picture and video in different file formats
- » Advanced functions for pictures processing (EDF, stitching, multi-fluorescence combine)
- » Powerful tools to perform measurements and generate custom reports

Laboratory



# B-510 Series

OPTIKA B-510 Series meets a wide variety of analysis applications, thanks to the comprehensive range of microscope models equipped with enhanced and impressive optics, a wide field of view of 22 mm, the state-of-the-art, exclusive X-LED lighting source and Koehler illuminator to produce high sample contrast and homogeneous bright light.

## A Perfect Downgrading of Top-Level Series


Many components of B-510 come from the B-810/1000 Series, the top-level in OPTIKA range, to ensure the state-of-the-art performance and at the same time an incredible level of reliability and durability. Its excellent quality/price ratio is achieved through an intelligent rationalization of production costs and choice of materials.

## X-LED<sup>3</sup> Exclusive Lighting Source

Special technology able to double the light intensity for incomparable performance, ensuring constant pure-white colour temperature (6,300K colour temperature).

Relevant money and energy saving thanks to the incredibly low energy consumptions which allows you to cut the electricity bills by 90%!

The electric consumption (3.6 W only) proves the high efficiency of this system: incredibly high light intensity combined with low consumption.

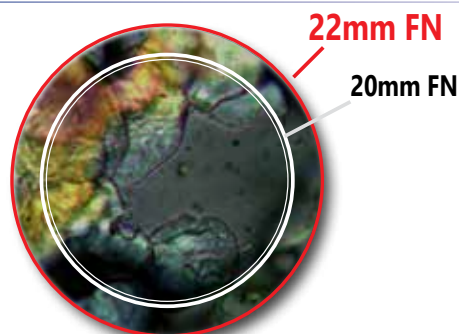

22mm FN

20mm FN

## Large Specimen View (22 mm Field Number)

The **F.O.V.** (field of view) is based on a comfortable diameter of 22 mm.

This means that an extra wide area of the sample can be inspected and allows a natural and easy view, particularly needed in a laboratory environment.

## Safe And Convenient Operations

Rounded edge rackless stage has been designed with a belt-driven mechanism that allows a smooth movement without any protruding part.

This design gives you a more compact solution and lowers any risk of injury after accidentally hitting the rack with your hands.

The electric consumption (3.6 W only) proves the high efficiency of this system: incredibly high light intensity combined with low consumption.



OPTIKA  
ITALY



# Advanced Routine Lab Upright Microscopes


## Universal Condenser For Brightfield, Darkfield & Phase

OPTIKA B-510 phase contrast microscopes are equipped with a 5-position dedicated rotating condenser for brightfield (standard use), phase contrast (10x/20x, 40x and 100x phase diaphragms), and a darkfield position for dry objectives.



## Exclusive X-LED<sup>3</sup> Darkfield Condenser

The special condenser with integrated, exclusive X-LED<sup>3</sup> illuminator replaces any other external and expensive lighting source required for these applications and is ideal for great-looking, rich and high-quality specimen view.

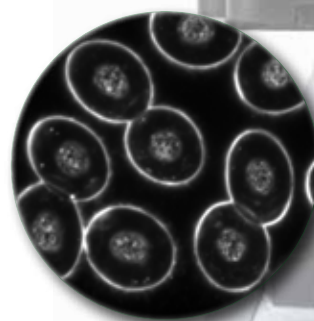

## In fluorescence we can offer several options.

According to your application and to the fluorochromes you are using, we can help you to identify the best light source.

### Traditional, HBO Fluorescence

- » The most used and diffused method, worldwide
- » Wide spectrum range for future upgrades

### Innovative, LED Fluorescence

- » Recommended for routine applications
- » Cost-effective, money saving technology
  - » Ready for immediate operation
  - » Eliminate warm-up/cool-down times
  - » Forget lamp replacement & centering



# B-510BF / B-510ERGO - Brightfield Microscope

Advanced routine laboratory microscope for brightfield observations with IOS W-PLAN objectives and rackless stage. The high-efficiency **X-LED<sup>3</sup>** makes it reliable for all transmitted light observations for great-looking, rich and high-quality view.



**B-510BF**




**B-510ERGO**

Part	Description
<b>Observation mode:</b>	Brightfield.
<b>Head:</b>	<b>B-510BF:</b> Trinocular (fixed 50/50), 30° inclined, 360° rotating. <b>B-510ERGO:</b> Binocular ergonomic head, 30° - 60° inclined, 360° rotating.
<b>Interpupillary distance:</b>	Adjustable between 50 and 75 mm.
<b>Dioptric adjustment:</b>	On the left eyepiece tube.
<b>Eyepieces:</b>	WF10x/22 mm, high eye-point and with rubber cups.
<b>Nosepiece:</b>	Quintuple revolving nosepiece, rotation on ball bearings.
<b>Objectives:</b>	IOS W-PLAN 4x/0.10 IOS W-PLAN 10x/0.25 IOS W-PLAN 40x/0.65 IOS W-PLAN 100x/1.25 (Oil) All with anti-fungus treatment.

Part	Description
<b>Specimen stage:</b>	Double layer rackless mechanical stage, 233x147 mm, 78x54 mm X-Y range.
<b>Focusing:</b>	Coaxial coarse (adjustable tension) and fine focusing mechanism with limit stop to prevent the contact between objective and specimen.
<b>Condenser:</b>	Swing-out N.A. 0.2/0.9, with iris diaphragm, focusable and centerable.
<b>Transmitted illumination (Full Koehler type):</b>	X-LED <sup>3</sup> with white 3.6 W LED (6,300K) with brightness control. Multi-plug 100-240Vac/6Vdc external power supply.

# B-510PH - Phase Contrast Microscope

Advanced routine laboratory microscope for brightfield, darkfield and phase contrast observations with IOS W-PLAN PH objectives and rackless stage. Especially dedicated to phase contrast observation, the microscope ensures a high image sharpness even with complex specimens. The high-efficiency **X-LED<sup>3</sup>** makes it reliable for all transmitted light observations.

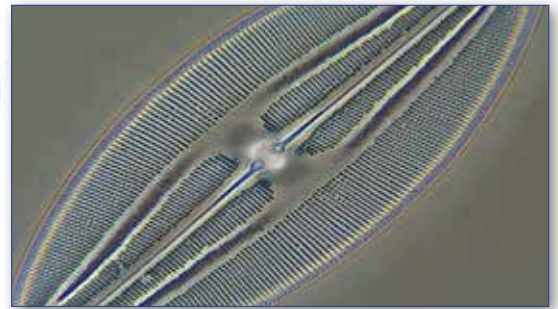


Part	Description
<b>Observation mode:</b>	Brightfield, phase contrast and darkfield (dry).
<b>Head:</b>	Trinocular (fixed 50/50), 30° inclined, 360° rotating.
<b>Interpupillary distance:</b>	Adjustable between 50 and 75 mm.
<b>Dioptric adjustment:</b>	On the left eyepiece tube.
<b>Eyepieces:</b>	WF10x/22 mm, high eye-point and with rubber cups.
<b>Nosepiece:</b>	Quintuple revolving nosepiece, rotation on ball bearings.
<b>Objectives:</b>	IOS W-PLAN PH 10x/0.25 IOS W-PLAN PH 20x/0.40 IOS W-PLAN PH 40x/0.65 IOS W-PLAN PH 100x/1.25 (Oil) All with anti-fungus treatment.

Part	Description
<b>Specimen stage:</b>	Double layer rackless mechanical stage, 233x147 mm, 78x54 mm X-Y range.
<b>Focusing:</b>	Coaxial coarse (adjustable tension) and fine focusing mechanism with limit stop to prevent the contact between objective and specimen.
<b>Condenser:</b>	Phase condenser (10x/20x, 40x, 100x) with darkfield (dry) and brightfield.
<b>Transmitted illumination (Full Koehler type):</b>	X-LED <sup>3</sup> with white 3.6 W LED (6,300K) with brightness control. Multi-plug 100-240Vac/6Vdc external power supply.

# B-510ASB - Asbestos Analysis Microscope

Advanced routine laboratory microscope for brightfield and phase contrast observations with IOS W-PLAN objectives and rackless stage. Ideal for Asbestos analysis in accordance to international rules with 12.5x eyepieces and Walton & Becket graticule to perform perfect asbestos fibers analysis at a glance. The high-efficiency **X-LED<sup>3</sup>** makes it reliable for all transmitted light observations.

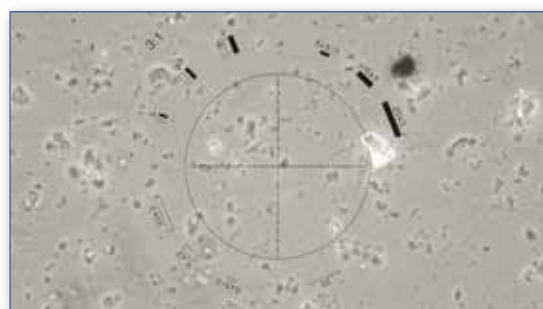


Part	Description
<b>Observation mode:</b>	Brightfield, phase contrast.
<b>Head:</b>	Trinocular (fixed 50/50), 30° inclined, 360° rotating.
<b>Interpupillary distance:</b>	Adjustable between 50 and 75 mm.
<b>Dioptric adjustment:</b>	On the left eyepiece tube.
<b>Eyepieces:</b>	WF10x/22 mm, high eye-point and WF12.5x/18 mm with dioptric adjustment, one with Walton & Beckett graticule.
<b>Nosepiece:</b>	Quintuple revolving nosepiece, rotation on ball bearings.
<b>Objectives:</b>	IOS W-PLAN 4x/0.10    IOS W-PLAN 10x/0.25 IOS W-PLAN PH 40x/0.65    IOS W-PLAN 100x/1.25 (Oil) All with anti-fungus treatment.

Part	Description
<b>Specimen stage:</b>	Double layer rackless mechanical stage, 233x147 mm, 78x54 mm X-Y range.
<b>Focusing:</b>	Coaxial coarse (adjustable tension) and fine focusing mechanism with limit stop to prevent the contact between objective and specimen.
<b>Condenser:</b>	Abbe N.A. 1.25, with objective-coded iris diaphragm, focusable and centerable. With 40x phase contrast slider.
<b>Transmitted illumination (Full Koehler type):</b>	X-LED <sup>3</sup> with white 3.6 W LED (6,300K) with brightness control. Multi-plug 100-240Vac/6Vdc external power supply.

# B-510DK - Immersion Darkfield Microscope

Advanced routine laboratory microscope for brightfield and darkfield observations with IOS W-PLAN objectives (including 100x with iris) and rackless stage for biology and especially darkfield fresh blood analysis and the exclusive **X-LED<sup>3</sup>** illumination system. The special condenser with integrated, exclusive X-LED<sup>3</sup> illuminator replaces any other external and expensive lighting source required for these applications and is ideal for great-looking, rich and high-quality specimen view. Our immersion darkfield system provides the same result achieved by 150W external illuminators in combination with traditional cardioid darkfield condenser.

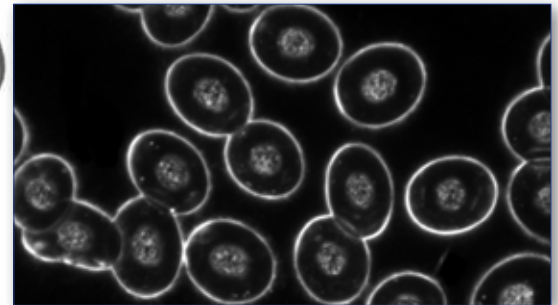


Part	Description
<b>Observation mode:</b>	Brightfield, oil immersion darkfield.
<b>Head:</b>	Trinocular (fixed 50/50), 30° inclined, 360° rotating.
<b>Interpupillary distance:</b>	Adjustable between 50 and 75 mm.
<b>Dioptric adjustment:</b>	On the left eyepiece tube.
<b>Eyepieces:</b>	WF10x/22 mm, high eye-point and with rubber cups.
<b>Nosepiece:</b>	Quintuple revolving nosepiece, rotation on ball bearings.
<b>Objectives:</b>	IOS W-PLAN 4x/0.10 IOS W-PLAN 10x/0.25 IOS W-PLAN 40x/0.65 IOS W-PLAN 100x/1.25 (oil) with iris All with anti-fungus treatment.

Part	Description
<b>Specimen stage:</b>	Double layer rackless mechanical stage, 233x147 mm, 78x54 mm X-Y range.
<b>Focusing:</b>	Coaxial coarse (adjustable tension) and fine focusing mechanism with limit stop to prevent the contact between objective and specimen.
<b>Brightfield condenser:</b>	Darkfield N.A. 1.36 (oil immersion) with built-in X-LED <sup>3</sup> .
<b>Transmitted illumination (Full Koehler type):</b>	X-LED <sup>3</sup> with white 3.6 W LED (6,300K) with brightness control. Multi-plug 100-240Vac/6Vdc external power supply.

# 2 B-510FL - HBO Fluorescence Microscope

Advanced routine laboratory microscope for brightfield and fluorescence observations with Semi-Apo IOS W-PLAN F objectives to enhance the visibility of the sample and increase the overall contrast. The **HBO fluorescence** illuminator provides an outstanding flexibility of use, standing the blue and green filter sets (supplied as standard) for Auramine, FITC, GFP and YFP (with blue filter set) plus Rhodamine, Texas Red and TRITC (with the green one), yet giving the possibility to combine any other specific filter sets for future upgrade. Transmitted light through the exclusive **X-LED<sup>3</sup>** to ensure great-looking, rich and high-quality specimen view.

-  22
- 
- 
- 
- 
- 
- 
- 

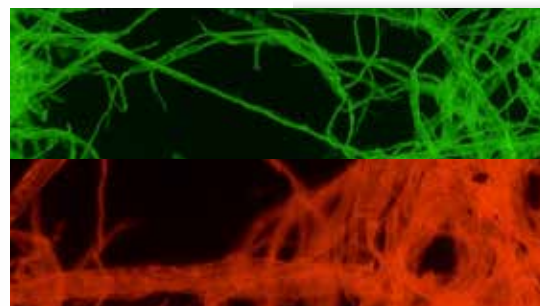

Standard filterset

Name	Excitation filter (nm)	Dichroic mirror cut-off (nm)	Emission filter (nm)
<b>B Blue</b>	460 – 490	505	515LP
<b>G Green</b>	510 – 550	570	590LP



Additional filterset (optional)

Name	Excitation filter (nm)	Dichroic mirror cut-off (nm)	Emission filter (nm)
<b>V (Violet)</b>	390 – 420	440	455LP
<b>UV</b>	325 – 375	415	435LP

Part	Description
<b>Observation mode:</b>	Brightfield, HBO fluorescence.
<b>Epi-illumination and filter:</b>	HBO 100 W high pressure mercury lamp. 4-position filter holder; blue & green included.
<b>Head:</b>	Trinocular (3-position 100/0, 50/50, 0/100), 30° inclined, 360° rotating.
<b>Interpupillary distance:</b>	Adjustable between 50 and 75 mm.
<b>Dioptric adjustment:</b>	On the left eyepiece tube.
<b>Eyepieces:</b>	WF10x/22 mm, high eye-point and with rubber cups.
<b>Nosepiece:</b>	Quintuple revolving nosepiece, rotation on ball bearings.
<b>Objectives:</b>	IOS W-PLAN F 4x/0.13      IOS W-PLAN F 10x/0.30 IOS W-PLAN F 20x/0.50    IOS W-PLAN F 40x/0.75 All with anti-fungus treatment.

Part	Description
<b>Specimen stage:</b>	Double layer rackless mechanical stage, 233x147 mm, 78x54 mm X-Y range.
<b>Focusing:</b>	Coaxial coarse (adjustable tension) and fine focusing mechanism with limit stop to prevent the contact between objective and specimen.
<b>Condenser:</b>	Swing-out N.A. 0.2/0.9, with iris diaphragm, focusable and centerable.
<b>Transmitted illumination (Full Koehler type):</b>	X-LED <sup>3</sup> with white 3.6 W LED (6,300K) with brightness control. Multi-plug 100-240Vac/6Vdc external power supply.

# B-510LD1 - LED Fluorescence Microscope

Advanced routine fluorescence microscope for transmitted brightfield and fluorescence observations with IOS W-PLAN objectives. The extremely powerful LED fluorescence illuminator is combined with blue excitation filter set for the visualization of the following fluorochromes: Acridine Yellow, Acridine Orange, Auramine, DiO, DTAF, FITC, GFP, YFP, etc. LED fluorescence ensures unparalleled convenience eliminating warm-up/cool-down times and all the inconveniences related lamp replacement and adjustment. Transmitted light through the exclusive **X-LED<sup>3</sup>** to ensure great-looking, rich and high-quality specimen view.

-  22
- 
- 
- 
- 
- 
- 
- 



Standard filterset

Name	Excitation filter (nm)	Dichroic mirror cut-off (nm)	Emission filter (nm)
B Blue	460 – 490	505	515LP


Part	Description
<b>Observation mode:</b>	Brightfield, LED fluorescence.
<b>Epi-illumination and filter:</b>	High-power blue LED with brightness control. 4-position filter holder; blue included.
<b>Head:</b>	Trinocular (3-position 100/0, 50/50, 0/100), 30° inclined, 360° rotating.
<b>Interpupillary distance:</b>	Adjustable between 50 and 75 mm.
<b>Dioptric adjustment:</b>	On the left eyepiece tube.
<b>Eyepieces:</b>	WF10x/22 mm, high eye-point and with rubber cups.
<b>Nosepiece:</b>	Quintuple revolving nosepiece, rotation on ball bearings.
<b>Objectives:</b>	IOS W-PLAN 4x/0.10      IOS W-PLAN 10x/0.25 IOS W-PLAN 40x/0.65    IOS W-PLAN 100x/1.25 (Oil) All with anti-fungus treatment.

Part	Description
<b>Specimen stage:</b>	Double layer rackless mechanical stage, 233x147 mm, 78x54 mm X-Y range.
<b>Focusing:</b>	Coaxial coarse (adjustable tension) and fine focusing mechanism with limit stop to prevent the contact between objective and specimen.
<b>Condenser:</b>	Swing-out N.A. 0.2/0.9, with iris diaphragm, focusable and centerable.
<b>Transmitted illumination (Full Koehler type):</b>	X-LED <sup>3</sup> with white 3.6 W LED (6,300K) with brightness control. Multi-plug 100-240Vac/6Vdc external power supply.

# B-510LD2 - LED Fluorescence Microscope

Advanced routine fluorescence microscope for transmitted brightfield and fluorescence observations with IOS W-PLAN objectives. The extremely powerful LED fluorescence illuminator is combined with blue and green excitation filter set for the visualization of the following fluorochromes: Acridine Yellow, Acridine Orange, Auramine, DiO, DTAF, FITC, GFP, YFP, etc. (blue) plus Rhodamine, Texas Red and TRITC (green). LED fluorescence ensures unparalleled convenience eliminating warm-up/cool-down times and all the inconveniences related lamp replacement and adjustment. Transmitted light through the exclusive **X-LED<sup>3</sup>** to ensure great-looking, rich and high-quality specimen view.

-  22
- 
- 
- 
- 
- 
- 
- 
- 

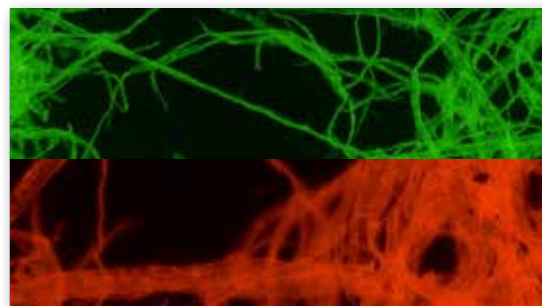

### Standard filterset

Name	Excitation filter (nm)	Dichroic mirror cut-off (nm)	Emission filter (nm)
<b>B Blue</b>	460 – 490	505	515LP
<b>G Green</b>	510 – 550	570	590LP

Part	Description
<b>Observation mode:</b>	Brightfield, LED fluorescence.
<b>Epi-illumination and filters:</b>	High-power wide spectrum LED with brightness control. 4-position filter holder; blue and green included.
<b>Head:</b>	Trinocular (3-position 100/0, 50/50, 0/100), 30° inclined, 360° rotating.
<b>Interpupillary distance:</b>	Adjustable between 50 and 75 mm.
<b>Dioptric adjustment:</b>	On the left eyepiece tube.
<b>Eyepieces:</b>	WF10x/22 mm, high eye-point and with rubber cups.
<b>Nosepiece:</b>	Quintuple revolving nosepiece, rotation on ball bearings.
<b>Objectives:</b>	IOS W-PLAN 4x/0.10      IOS W-PLAN 10x/0.25 IOS W-PLAN 40x/0.65    IOS W-PLAN 100x/1.25 (Oil) All with anti-fungus treatment.


Part	Description
<b>Specimen stage:</b>	Double layer rackless mechanical stage, 233x147 mm, 78x54 mm X-Y range.
<b>Focusing:</b>	Coaxial coarse (adjustable tension) and fine focusing mechanism with limit stop to prevent the contact between objective and specimen.
<b>Condenser:</b>	Swing-out N.A. 0.2/0.9, with iris diaphragm, focusable and centerable.
<b>Transmitted illumination (Full Koehler type):</b>	X-LED <sup>3</sup> with white 3.6 W LED (6,300K) with brightness control. Multi-plug 100-240Vac/6Vdc external power supply.



# B-510POL - Polarizing Microscope

Advanced routine laboratory microscope for transmitted light in brightfield and polarized light observations with strain-free IOS W-PLAN POL objectives. Complete of polarizer and analyzer filters, Bertrand lens for conoscopic observation, compensator plates and high-precision rotatable stages. It comes with the exclusive **X-LED<sup>3</sup>** illumination system to deliver bright and clear images, along with all the accessories to perform accurate polarization analysis in biology and materials science.

-  22
- 
-  X-LED<sup>3</sup>
- 
-  IOS
-  ∞
-  W-PLAN
-  POL

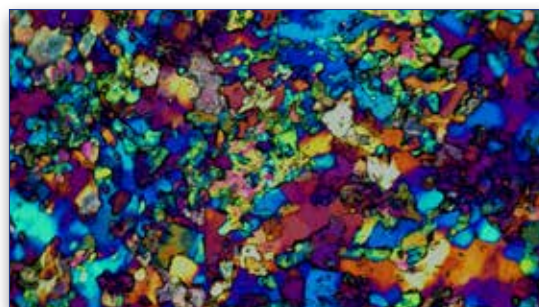


Part	Description
<b>Observation mode:</b>	Brightfield, transmitted polarized light and conoscopy.
<b>Bertrand lens and polarizing attachment:</b>	Swing-out type with centering mechanism for observation in conoscopy/orthoscopy. Rotatable analyzer from 0° to 90° with graduated scale. Tint plates: 1° order red ( $\lambda$ ); $\lambda/4$ ; Quartz wedge.
<b>Head:</b>	Trinocular (fixed 50/50), 30° inclined, 360° rotating.
<b>Interpupillary distance:</b>	Adjustable between 50 and 75 mm.
<b>Dioptric adjustment:</b>	On the left eyepiece tube.
<b>Eyepieces:</b>	WF10x/22 mm, high eye-point and with rubber cups. One with crosshair.
<b>Nosepiece:</b>	Quadruple revolving nosepiece, rotation on ball bearings. Centering system for each objective.

Part	Description
<b>Objectives (strain-free):</b>	IOS W-PLAN POL 4x/0.10    IOS W-PLAN POL 10x/0.25 IOS W-PLAN POL 20x/0.45    IOS W-PLAN POL 40x/0.65 All with anti-fungus treatment.
<b>Specimen stage:</b>	Rotatable stage with locking mechanism and centering knobs. Vernier scale with accuracy 0.1 mm. Diameter 145 mm. Specimen slide clamps.
<b>Focusing:</b>	Coaxial coarse (adjustable tension) and fine focusing mechanism with limit stop to prevent the contact between objective and specimen.
<b>Condenser:</b>	Swing-out N.A. 0.2/0.9, with iris diaphragm, focusable and centerable. With rotating polarizing filter.
<b>Transmitted illumination (Full Koehler type):</b>	X-LED <sup>3</sup> with white 3.6 W LED (6.300 K) with brightness control. Multi-plug 100-240Vac/6Vdc external power supply.

# B-510POL-I - Polarizing Microscope

Advanced routine laboratory microscope for brightfield and polarized light observations in transmitted and incident light with strain-free IOS LWD W-PLAN POL objectives. Complete of polarizer and analyzer filters, Bertrand lens for conoscopic observation, compensator plates and high-precision rotatable stages. It comes with the exclusive **X-LED<sup>3</sup>** illumination system to deliver bright and clear images, along with all the accessories to perform accurate polarization analysis in biology and materials science.

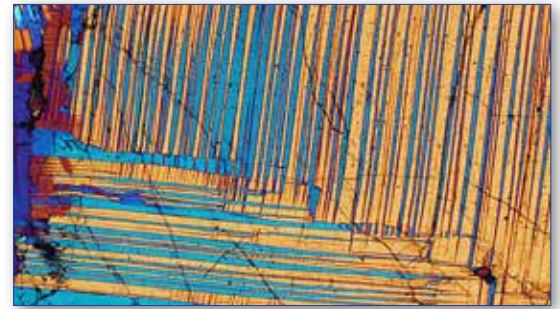

## Incident/transmitted light Objectives included

### Description

IOS LWD W-PLAN POL 5x/0.12, W.D. 15.5 mm

IOS LWD W-PLAN POL 10x/0.25, W.D. 10.0 mm

IOS LWD W-PLAN POL 20x/0.40, W.D. 5.8 mm









IOS LWD W-PLAN POL 50x/0.75, W.D. 0.32 mm



Part	Description
<b>Observation mode:</b>	Brightfield, transmitted/incident polarized light and conoscopy.
<b>Epi-illumination and filters:</b>	X-LED <sup>3</sup> with white 8 W LED (6.300 K) with brightness control. With polarizer and rotating analyzer for incident illumination, aperture and field diaphragm. With additional filter holder.
<b>Bertrand lens and polarizing attachment:</b>	Swing-out type with centering mechanism for observation in conoscopy/orthoscopy. Rotatable analyzer from 0° to 90° with graduated scale. Tint plates: 1° order red ( $\lambda$ ); $\lambda/4$ ; Quartz wedge.
<b>Head:</b>	Trinocular (fixed 50/50), 30° inclined, 360° rotating.
<b>Interpupillary distance:</b>	Adjustable between 50 and 75 mm.
<b>Dioptric adjustment:</b>	On the left eyepiece tube.
<b>Eyepieces:</b>	WF10x/22 mm, high eye-point and with rubber cups. One with crosshair.
<b>Nosepiece:</b>	Quadruple revolving nosepiece, rotation on ball bearings. Centering system for each objective.

Part	Description
<b>Objectives (strain-free):</b>	IOS LWD W-PLAN POL 5x/0.12 IOS LWD W-PLAN POL 10x/0.25 IOS LWD W-PLAN POL 20x/0.40 IOS LWD W-PLAN POL 50x/0.75 All with anti-fungus treatment.
<b>Specimen stage:</b>	Rotatable stage with locking mechanism and centering knobs. Vernier scale with accuracy 0.1 mm. Diameter 145 mm. Specimen slide clamps.
<b>Focusing:</b>	Coaxial coarse (adjustable tension) and fine focusing mechanism with limit stop to prevent the contact between objective and specimen.
<b>Condenser:</b>	Swing-out N.A. 0.2/0.9, with iris diaphragm, focusable and centerable. With rotating polarizing filter.
<b>Transmitted illumination (Full Koehler type):</b>	X-LED <sup>3</sup> with white 3.6 W LED (6.300 K) with brightness control. Multi-plug 100-240Vac/6Vdc external power supply.

# B-510MET - Metallurgical Microscope

Advanced routine laboratory microscope with IOS W-PLAN MET objectives and metallurgical attachment with the exclusive **X-LED<sup>3</sup>** lighting source for incident illumination only. The NCG (no cover glass) objectives are especially designed for microscopy use without a cover slip ideal for metallographic samples and other opaque specimens.

-  22
- 
- 
- 
- 
- 
- 
- 

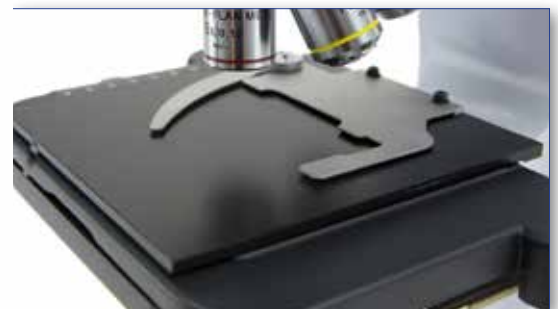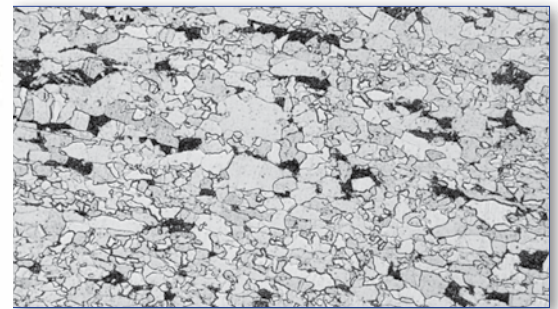

Part	Description
<b>Observation mode:</b>	Brightfield, simple polarized light, oblique illumination on incident light.
<b>Epi-illumination and polarizing filters:</b>	X-LED <sup>3</sup> with white 8 W LED (6.300 K) with brightness control. With aperture and field diaphragms, and oblique illumination system. With polarizer and analyzer. Multi-plug 100-240Vac/6Vdc external power supply.
<b>Head:</b>	Trinocular (fixed 50/50), 30° inclined, 360° rotating.
<b>Interpupillary distance:</b>	Adjustable between 50 and 75 mm.
<b>Dioptric adjustment:</b>	On the left eyepiece tube.
<b>Eyepieces:</b>	WF10x/22 mm, high eye-point and with rubber cups.
<b>Nosepiece:</b>	Quintuple revolving nosepiece, rotation on ball bearings.

Part	Description
<b>Objectives (strain-free):</b>	IOS W-PLAN MET 5x/0.12 IOS W-PLAN MET 10x/0.25 IOS W-PLAN MET 20x/0.40 IOS W-PLAN MET 50x/0.75 All with anti-fungus treatment.
<b>Specimen stage:</b>	Double layer rackless mechanical stage, 233x147 mm, 78x54 mm X-Y range.
<b>Focusing:</b>	Coaxial coarse (adjustable tension) and fine focusing mechanism with limit stop to prevent the contact between objective and specimen.

# B-510METR - Metallurgical Microscope

Advanced routine laboratory microscope with IOS W-PLAN MET objectives and metallurgical attachment with the exclusive **X-LED<sup>3</sup>** lighting source for both transmitted and incident illumination. The NCG (no cover glass) objectives are especially designed for microscopy use without a cover slip ideal for metallographic samples and other opaque specimens.



Part	Description
<b>Observation mode:</b>	Brightfield on transmitted light. Brightfield, simple polarized light, oblique illumination on incident light.
<b>Epi-illumination and polarizing filters:</b>	X-LED <sup>3</sup> with white 8 W LED (6.300 K) with brightness control. With aperture and field diaphragms, and oblique illumination system. With polarizer and analyzer.
<b>Head:</b>	Trinocular (fixed 50/50), 30° inclined, 360° rotating.
<b>Interpupillary distance:</b>	Adjustable between 50 and 75 mm.
<b>Dioptric adjustment:</b>	On the left eyepiece tube.
<b>Eyepieces:</b>	WF10x/22 mm, high eye-point and with rubber cups.
<b>Nosepiece:</b>	Quintuple revolving nosepiece, rotation on ball bearings.

Part	Description
<b>Objectives (strain-free):</b>	IOS W-PLAN MET 5x/0.12 IOS W-PLAN MET 10x/0.25 IOS W-PLAN MET 20x/0.40 IOS W-PLAN MET 50x/0.75 All with anti-fungus treatment.
<b>Specimen stage:</b>	Double layer rackless mechanical stage, 233x147 mm, 78x54 mm X-Y range. With tempered glass plate.
<b>Focusing:</b>	Coaxial coarse (adjustable tension) and fine focusing mechanism with limit stop to prevent the contact between objective and specimen.
<b>Condenser:</b>	Swing-out N.A. 0.2/0.9, with iris diaphragm, focusable and centerable.
<b>Transmitted illumination (Full Koehler type):</b>	X-LED <sup>3</sup> with white 3.6 W LED (6.300 K) with brightness control. Multi-plug 100-240Vac/6Vdc external power supply.

# B-510 - Discussion Microscopes

Advanced routine laboratory microscope for brightfield observations with IOS W-PLAN objectives and rackless stage. Ideal for discussion groups and teaching purpose for multiple observers, up to five users simultaneously. A three-color LED pointer facilitates the indication and identification of the object observed. The high-efficiency **X-LED<sup>3</sup>** makes it reliable for all transmitted light observations for great-looking, rich and high-quality view.



**B-510-2F**



**B-510-2**



**B-510-3**



**B-510-5**

Part	Description
<b>Observation mode:</b>	Brightfield
<b>Head:</b>	Trinocular (fixed photo port 50/50), 30° inclined, 360° rotating.
<b>Interpupillary distance:</b>	Adjustable between 50 and 75 mm.
<b>Dioptric adjustment:</b>	On the left eyepiece tube.
<b>Eyepieces:</b>	Main head: WF10x/22 mm, high eye-point and with rubber cups. Additional head(s): WF10x/20 mm, high eye-point.
<b>Nosepiece:</b>	Quintuple revolving nosepiece, rotation on ball bearings.
<b>Objectives:</b>	IOS W-PLAN 4x/0.10      IOS W-PLAN 10x/0.25 IOS W-PLAN 40x/0.65    IOS W-PLAN 100x/1.25 (Oil) All with anti-fungus treatment.

Part	Description
<b>Specimen stage:</b>	Double layer rackless mechanical stage, 233x147 mm, 78x54 mm X-Y range.
<b>Focusing:</b>	Coaxial coarse (adjustable tension) and fine focusing mechanism with limit stop to prevent the contact between objective and specimen.
<b>Condenser:</b>	Swing-out N.A. 0.2/0.9, with iris diaphragm, focusable and centerable.
<b>Transmitted illumination (Full Koehler type):</b>	X-LED <sup>3</sup> with white 3.6 W LED (6,300K) with brightness control. Multi-plug 100-240Vac/6Vdc external power supply.

# B-510 Series - Comparison chart

Model	Head	Eyepieces	Nosepiece	Attachment	Objectives
<b>B-510BF</b>	Trinocular (50/50), 30° inclined, 360° rotating	WF10x/22mm, high eye-point	Quintuple, reversed	-	IOS W-PLAN 4x, 10x, 40x, 100x (oil)
<b>B-510ERGO</b>	Binocular ergonomical, 30°- 60° inclined 360° rotating	WF10x/22mm, high eye-point	Quintuple, reversed	-	IOS W-PLAN 4x, 10x, 40x, 100x (oil)
<b>B-510PH</b>	Trinocular (50/50), 30° inclined, 360° rotating	WF10x/22mm, high eye-point	Quintuple, reversed	-	IOS W-PLAN PH 10x, 20x, 40x, 100x (oil)
<b>B-510ASB</b>	Trinocular (50/50), 30° inclined, 360° rotating	WF10x/22mm, high eye-point WF12.5x/18mm w/W&B reticle	Quintuple, reversed	-	IOS W-PLAN 4x, 10x, 40xPH, 100x (oil)
<b>B-510DK</b>	Trinocular (50/50), 30° inclined, 360° rotating	WF10x/22mm, high eye-point	Quintuple, reversed	-	IOS W-PLAN 4x, 10x, 40x, 100x with iris diaphragm (oil)
<b>B-510FL</b>	Trinocular (100/0, 50/50, 0/100), 30° inclined, 360° rotating	WF10x/22mm, high eye-point	Quintuple, reversed	Epi-Florescence attachment, with 4-position filterset slider. Equipped with Blue (FITC) and Green (TRITC) filtersets	IOS W-PLAN F 4x, 10x, 20x, 40x (oil)
<b>B-510LD1</b>	Trinocular (3-position 100/0, 50/50, 0/100), 30° inclined, 360° rotating.	WF10x/22mm, high eye-point	Quintuple, reversed	Epi-Florescence attachment, with 3-position filterset slider. Equipped with Blue filterset (FITC)	IOS W-PLAN 4x, 10x, 40x, 100x (oil)
<b>B-510LD2</b>	Trinocular (3-position 100/0, 50/50, 0/100), 30° inclined, 360° rotating.	WF10x/22mm, high eye-point	Quintuple, reversed	Epi-Florescence attachment, with 3-position filterset slider. Equipped with Blue (FITC) and Green (TRITC) filtersets	IOS W-PLAN 4x, 10x, 40x, 100x (oil)
<b>B-510POL</b>	Trinocular (50/50), 30° inclined, 360° rotating	WF10x/22mm, high eye-point	Quadruple, reversed. Objective positions centrabale.	Swing-out Bertrand lens with centering mechanism for observation in conoscopy/orthoscopy. Rotatable analyzer from 0° to 90° with graduated scale. Tint plates: 1° order red ( $\lambda$ ); $\lambda/4$ ; Quartz wedge	IOS W-PLAN POL 4x, 10x, 20x, 40x
<b>B-510POL-I</b>	Trinocular (50/50), 30° inclined, 360° rotating	WF10x/22mm, high eye-point	Quadruple, reversed. Objective positions centrabale.	Incident light attachment with Polarizer for incident illumination, with Aperture & Field diaphragms and additional filter holder. Swing-out Bertrand lens with centering mechanism for observation in conoscopy/orthoscopy. Rotatable analyzer from 0° to 90° with graduated scale. Tint plates: 1° order red ( $\lambda$ ); $\lambda/4$ ; Quartz wedge	IOS LWD W-PLAN POL 5x, 10x, 20x, 50x
<b>B-510MET</b>	Trinocular (50/50), 30° inclined, 360° rotating	WF10x/22mm, high eye-point	Quintuple, reversed	Incident light attachment with Polarizer and rotating Analyzer for incident illumination, with Aperture & Field diaphragms and 2 additional filter holders. Oblique illumination	IOS W-PLAN MET 5x, 10x, 20x, 50x
<b>B-510METR</b>	Trinocular (50/50), 30° inclined, 360° rotating	WF10x/22mm, high eye-point	Quintuple, reversed	Incident light attachment with Polarizer and rotating Analyzer for incident illumination, with Aperture & Field diaphragms and 2 additional filter holders; Epi/Transmitted light selector. Oblique illumination	IOS W-PLAN MET 5x, 10x, 20x, 50x
<b>B-510-2F</b>	Trinocular (50/50), 30° inclined, 360° rotating	WF10x/22mm, high eye-point	Quintuple, reversed	Discussion bridge for 2 observers , Face-to-Face type. 2nd binocular head with WF10x/20mm eyepieces. Equipped with RGB discussion pointer	IOS W-PLAN 4x, 10x, 40x, 100x (oil)
<b>B-510-2</b>	Trinocular (50/50), 30° inclined, 360° rotating	WF10x/22mm, high eye-point	Quintuple, reversed	Discussion bridge for 2 observers , Side-by-Side type. 2nd binocular head with WF10x/20mm eyepieces. Equipped with RGB discussion pointer	IOS W-PLAN 4x, 10x, 40x, 100x (oil)
<b>B-510-3</b>	Trinocular (50/50), 30° inclined, 360° rotating	WF10x/22mm, high eye-point	Quintuple, reversed	Discussion bridge for 3 observers. Additional binocular heads with WF10x/20mm eyepieces. Equipped with RGB discussion pointer	IOS W-PLAN 4x, 10x, 40x, 100x (oil)
<b>B-510-5</b>	Trinocular (50/50), 30° inclined, 360° rotating	WF10x/22mm, high eye-point	Quintuple, reversed	Discussion bridge for 5 observers. Additional binocular heads with WF10x/20mm eyepieces. Equipped with RGB discussion pointer	IOS W-PLAN 4x, 10x, 40x, 100x (oil)

# B-510 Series - Comparison chart

Stage	Focusing	Condenser	Incident Illumination	Transmitted Illumination
Double layer, 233x147 mm, moving range 78x54 mm, X-axis rackless	Coaxial coarse and fine, limit stop, adjustable tension	Swing-out type, sliding-in, N.A. 0.2/0.9, with centering system	-	X-LED <sup>3</sup> with white 3.6 W LED (6,300K), brightness control. Full Koehler type.
Double layer, 233x147 mm, moving range 78x54 mm, X-axis rackless	Coaxial coarse and fine, limit stop, adjustable tension	Swing-out type, sliding-in, N.A. 0.2/0.9, with centering system	-	X-LED <sup>3</sup> with white 3.6 W LED (6,300K), brightness control. Full Koehler type.
Double layer, 233x147 mm, moving range 78x54 mm, X-axis rackless	Coaxial coarse and fine, limit stop, adjustable tension	Phase condenser (10x/20x, 40x, 100x) with darkfield (dry) and brightfield	-	X-LED <sup>3</sup> with white 3.6 W LED (6,300K), brightness control. Full Koehler type.
Double layer, 233x147 mm, moving range 78x54 mm, X-axis rackless	Coaxial coarse and fine, limit stop, adjustable tension	Abbe N.A. 1.25, with objective-coded iris diaphragm, focusable and centerable. With 40x phase contrast slider.	-	X-LED <sup>3</sup> with white 3.6 W LED (6,300K), brightness control. Full Koehler type.
Double layer, 233x147 mm, moving range 78x54 mm, X-axis rackless	Coaxial coarse and fine, limit stop, adjustable tension	Swing-out type, sliding-in, N.A. 0.2/0.9, with centering system. Additional darkfield condenser, N.A. 1.36, built-in X-LED <sup>3</sup>	-	X-LED <sup>3</sup> with white 3.6 W LED (6,300K), brightness control. Full Koehler type.
Double layer, 233x147 mm, moving range 78x54 mm, X-axis rackless	Coaxial coarse and fine, limit stop, adjustable tension	Swing-out type, sliding-in, N.A. 0.2/0.9, with centering system	High Pressure HBO 100 W mercury bulb	X-LED <sup>3</sup> with white 3.6 W LED (6,300K), brightness control. Full Koehler type.
Double layer, 233x147 mm, moving range 78x54 mm, X-axis rackless	Coaxial coarse and fine, limit stop, adjustable tension	Swing-out type, sliding-in, N.A. 0.2/0.9, with centering system	High-power blue LED with brightness control	X-LED <sup>3</sup> with white 3.6 W LED (6,300K), brightness control. Full Koehler type.
Double layer, 233x147 mm, moving range 78x54 mm, X-axis rackless	Coaxial coarse and fine, limit stop, adjustable tension	Swing-out type, sliding-in, N.A. 0.2/0.9, with centering system	High-power wide spectrum LED with brightness control	X-LED <sup>3</sup> with white 3.6 W LED (6,300K), brightness control. Full Koehler type.
Rotating stage with locking mechanism and centering knobs. Vernier scale with accuracy 0.1 mm. Diameter 145 mm; Specimen slide clamps	Coaxial coarse and fine, limit stop, adjustable tension	Swing-out type, sliding-in, N.A. 0.2/0.9, with centering system. With rotating polarizing filter	-	X-LED <sup>3</sup> with white 3.6 W LED (6,300K), brightness control. Full Koehler type.
Rotating stage with locking mechanism and centering knobs. Vernier scale with accuracy 0.1 mm. Diameter 145 mm; Specimen slide clamps	Coaxial coarse and fine, limit stop, adjustable tension	Swing-out type, sliding-in, N.A. 0.2/0.9, with centering system. With rotating polarizing filter	X-LED <sup>3</sup> with white 8 W LED (6,300K), brightness control	X-LED <sup>3</sup> with white 3.6 W LED (6,300K), brightness control. Full Koehler type.
Double layer, 233x147 mm, moving range 78x54 mm, X-axis rackless; with metal plate for metallurgical samples	Coaxial coarse and fine, limit stop, adjustable tension	-	X-LED <sup>3</sup> with white 8 W LED (6,300K), brightness control	-
Double layer, 233x147 mm, moving range 78x54 mm, X-axis rackless; with glass plate for metallurgical samples	Coaxial coarse and fine, limit stop, adjustable tension	Swing-out type, sliding-in, N.A. 0.2/0.9, with centering system	X-LED <sup>3</sup> with white 8 W LED (6,300K), brightness control	X-LED <sup>3</sup> with white 3.6 W LED (6,300K), brightness control. Full Koehler type.
Double layer, 233x147 mm, moving range 78x54 mm, X-axis rackless	Coaxial coarse and fine, limit stop, adjustable tension	Swing-out type, sliding-in, N.A. 0.2/0.9, with centering system	-	X-LED <sup>3</sup> with white 3.6 W LED (6,300K), brightness control. Full Koehler type.
Double layer, 233x147 mm, moving range 78x54 mm, X-axis rackless	Coaxial coarse and fine, limit stop, adjustable tension	Swing-out type, sliding-in, N.A. 0.2/0.9, with centering system	-	X-LED <sup>3</sup> with white 3.6 W LED (6,300K), brightness control. Full Koehler type.
Double layer, 233x147 mm, moving range 78x54 mm, X-axis rackless	Coaxial coarse and fine, limit stop, adjustable tension	Swing-out type, sliding-in, N.A. 0.2/0.9, with centering system	-	X-LED <sup>3</sup> with white 3.6 W LED (6,300K), brightness control. Full Koehler type.
Double layer, 233x147 mm, moving range 78x54 mm, X-axis rackless	Coaxial coarse and fine, limit stop, adjustable tension	Swing-out type, sliding-in, N.A. 0.2/0.9, with centering system	-	X-LED <sup>3</sup> with white 3.6 W LED (6,300K), brightness control. Full Koehler type.

# B-510 Series - Accessories and parts

M-780	WF10x/22mm Eyepiece
M-601	WF15x/16mm Eyepiece
M-781	WF10x/22mm Micrometer Eyepiece
M-1004.N	Centering Telescope
M-1125	IOS W-PLAN Objective 4x/0.10
M-1126	IOS W-PLAN Objective 10x/0.25
M-1127	IOS W-PLAN Objective 20x/0.40
M-1128	IOS W-PLAN Objective 40x/0.65
M-1129	IOS W-PLAN Objective 60x/0.80
M-1130	IOS W-PLAN Objective 100x/1.25 (Oil immersion)
M-1130.1	IOS W-PLAN Objective 100x/1.25 with Iris Diaphragm (Oil imm.)
M-1120.N	IOS W-PLAN Phase Contrast Objective 10x/0.25
M-1121.N	IOS W-PLAN Phase Contrast Objective 20x/0.40
M-1122.N	IOS W-PLAN Phase Contrast Objective 40x/0.65
M-1123.N	IOS W-PLAN Phase Contrast Objective 100x/1.25 (Oil imm.)
M-1060	IOS W-PLAN F Semi-APO Objective 4x/0.13
M-1061	IOS W-PLAN F Semi-APO Objective 10x/0.30
M-1062	IOS W-PLAN F Semi-APO Objective 20x/0.50
M-1063	IOS W-PLAN F Semi-APO Objective 40x/0.75
M-1064	IOS W-PLAN F Semi-APO Objective 100x/1.30 (Oil immersion)
M-336	IOS W-PLAN MET Objective 5x/0.12
M-338	IOS W-PLAN MET Objective 10x/0.25
M-339	IOS W-PLAN MET Objective 20x/0.40
M-335	IOS W-PLAN MET Objective 50x/0.75
M-698.2	IOS W-PLAN MET Objective 100x/0.80 (Dry) - Suitable for Incident POL Applications
M-1131	IOS W-PLAN POL Objective 4x/0.10
M-1132	IOS W-PLAN POL Objective 10x/0.25
M-1133	IOS W-PLAN POL Objective 20x/0.45
M-1134	IOS W-PLAN POL Objective 40x/0.65
M-1135	IOS W-PLAN POL Objective 60x/0.80
M-1136	IOS LWD W-PLAN POL Objective 5x/0.12
M-1137	IOS LWD W-PLAN POL Objective 10x/0.25
M-1138	IOS LWD W-PLAN POL Objective 20x/0.40
M-1139	IOS LWD W-PLAN POL Objective 50x/0.75

M-1124.NO Phase contrast condenser, with phase rings 10x/20x and 40x



M-181	5-Position Phase Contrast Set, 10x-20x, 40x, 100x, BF, DF
M-185	DF condenser for dry objectives
M-636	Simple Polarizing Set (Polarizer and Analyser)
M-175.1	Rotating table for polarising set (For all models with 233x147mm reckless stage).

M-1037 Gout Analysis Kit



M-635 Heating stage, with digital temperature controller (only on newly purchased microscopes)



M-975	Blue Filter
M-977	Green Filter
M-979	Yellow Filter
M-989	Frosted Glass Filter
M-637	Fluorescence Filterset V (Filterblock not needed)
M-638	Fluorescence Filterset UV (Filterblock not needed)
M-699	Universal Tube Adapter
M-173	Photo adapter for APS-C and Full Frame Reflex cameras. To be used in combination with M-699 only.
M-620	0.35x Focusable C-Mount adapter for 1/3" sensor
M-620.1	0.5x Focusable C-Mount adapter for 1/2" sensor
M-620.2	0.65x Focusable C-Mount adapter for 2/3" sensor
M-620.3	1x Focusable C-Mount adapter for 1" sensor
M-005	Micrometer slide for software calibration, 1mm/10um, 10mm/100um
M-690	Eyecups (Pair)
M-151	HBO100W High-Pressure Mercury Bulb for Fluorescence
DC-003	TNT dust cover, medium – 600(l)x550(h) mm
15008	OPTIKA immersion oil 10ml
VP-510	IQ/OQ/PQ Validation Protocols.
15104	Cleaning kit



v 1.3.0 - OPTIKA reserves the right to make corrections, modifications, enhancements, improvements and other changes to its products at any time without notice.

## Headquarters and Manufacturing Facilities

**OPTIKA® S.r.l.** Via Rigla, 30 - 24010 Ponteranica (BG) - ITALY - Tel.: +39 035.571.392 - info@optikamicroscopes.com

## Optika Sales branches

**OPTIKA® Spain** spain@optikamicroscopes.com  
**OPTIKA® China** china@optikamicroscopes.com  
**OPTIKA® India** india@optikamicroscopes.com

**OPTIKA® USA** usa@optikamicroscopes.com  
**OPTIKA® Central America** camerica@optikamicroscopes.com